

USER'S MANUAL



2640 2.0GHz RF Field Strength Analyzer



Danger statements identify condition or practices that could result in injury or loss of life.



Caution statements identify conditions or practices that could result in damage or fire.



Ground statements identify conditions or practices that could connect protective conductor.

Caution for safety

• Prohibiting to removal the cover



Do not remove the instrument cover to access the internal components. Only B&K Precisions' Service technician with knowledge of the instruments' condition and dangerous voltages can repair the instrument.

Instruments that appear damaged or defective should be made inoperative and secured against unintended operation until they can be repaired by qualified service personnel.

• Keep the clean on power insert



Instrument's power insert should remain dust free.

Clean the power insert regularly. Dust could result in damage to this instrument.

Continually clean the dust on input terminal of RF frequency counter.

Clean the input terminal regularly. Dust could result in damage to the instrument.

RF in/output rating



Rating of RF input and output connector Maximum DC voltage rating RF input connector (socket): N type female, 50Ohms Maximum RF input power: 5Vrms Caution: Do not use over 5Vrms supplied and/or (-) power could result in damage to this

instrument

Do not operate this instrument if there is any doubt it is functioning properly: if operating personnel feels the instrument is not operating properly, return this instrument to B&K Precision for service and repair to ensure the safety features are maintained.



The operating Personnel must use the DC adaptor supplied with this instrument. Other adaptors could result in damage to this instrument and it is the limitation of warranty Exterior DC input connector should be matched with polar. DC connector tip must attach with (+) polar grounding.

The operating personnel must use grounded power Restore this instrument

• Instrument care



- * Avoid direct light
- * Keep away the heating system
- * Avoid high temperature (Ex. Inside of the car during the summer time)
- * Keep away from liquids
- * Avoid high moisture and/or poor ventilation
- * Keep away from dust and/or smoke
- * Avoid extremely low temperature

B&K Precision 2640 Ni-MH battery is rechargeable. Charging is controlled from the power of the battery cell and the temperature of the battery. Ni-MH Rechargeable battery is going to increase temp slowly until the temperature is extremely higher. Battery charging is finished automatically by checking the degree of the temperature (dT/dt). For battery protection, when the power of Battery cell is increased, comparing regular temperature and/or exterior temperature degree of when the temperature increases over 50 degrees, battery charging will be finished automatically.

Operating personnel must use Ni-MH Rechargeable Battery and do not operate in an explosive atmosphere.

- The battery usage time can change due to the using term, environment and temperature.
- When battery consumption is large battery-running time will decrease.

Operating personnel should phase in a new battery when battery-running time is less than half of the initial operating time.

- Operating personnel should not use this instrument and/or keep the battery in place for long periods of time, which could result in discharge of the battery.
- To avoid damages to battery, when battery is low, this instrument will turn off automatically.

Limited One-Year Warranty

B&K Precision warrants to the original purchaser that its products and the component parts thereof, will be free from defects in workmanship and materials for a period of one year from date of purchase from an authorized B&K Precision distributor.

B&K Precision will, without charge, repair or replace, at its option, defective product or component parts. Returned product must be accompanied by proof of the purchase date in the form of a sales receipt.

To obtain warranty coverage in the U.S.A., this product must be registered by completing the warranty registration form on www.bkprecision.com within fifteen (15) days of purchase.

Exclusions: This warranty does not apply in the event of misuse or abuse of the product or as a result of unauthorized alterations or repairs. The warranty is void if the serial number is altered, defaced or removed.

B&K Precision shall not be liable for any consequential damages, including without limitation damages resulting from loss of use. Some states do not allow limitations of incidental or consequential damages. So the above limitation or exclusion may not apply to you.

This warranty gives you specific rights and you may have other rights, which vary from state-to-state.

B&K Precision 22820 Savi Ranch Parkway Yorba Linda, CA 92887 www.bkprecision.com

Accessories (included)



Table of contents

1. Introduction
Overview11
2. Features
Main features12
3. Functions
RF Field Strength Analyzer13
Frequency Counter13
Specifications14
4. Instrument overview
Front Panel18
Rear Panel
Side Panel21
Top Panel22
5. Basic operation
Before Power On23
Power On24
Turn on Power of Instrument25
Description of operation screen26
Reception Mode32
Sweep Mode
Set up Span34
Frequency Input
Adjust Screen Level37
Run - Scanning
Marker
Power Meter46
Setting of attenuator49
LCD Light
LCD Contrast51
Buzzer ON/OFF52

Save/Load	53
Frequency Counter	57
Power Source	59
Level Unit	60
Reset	61
Baud Rate	62
Connection for PC	63
Auto Power	64
Offset	65
Menu	66
System	70

6. Description of key operating

Run [GHz]	73
Mode [MHz]	73
Sweep [kHz]	74
Marker [DEL]	74
No. 1 [Start/Stop]	75
No. 2 [Span]	75
No. 3 [Level]	76
No. 4 [Single]	76
No. 5 [Multi]	77
No. 6 [UNIT]	77
No. 7 [LCD Light]	78
No. 8 [LCD CONT; LCD Contrast]	78
No. 9 [Attenuator]	79
No. 0 [system]	79
Shift	80
Dot [Buzzer]	80
Menu [Load]	81
Enter [Save]	81
Up/Down Keys and Knob Key	82

Introduction (section 1)

Overview

The B&K Precision 2640 handheld RF Field Strength Analyzer is optimized to analyze signals from many different source for multiple applications. The B&K Precision 2640 has adopted a synthesizer method and has a wideband reception range of 100 kHz to 2,000 MHz. The characteristic of frequency response of the B&K Precision 2640 is calculated by memorized calculation data from a "look up table", and so it enables the B&K Precision 2640 to measure accurate levels and make easy analysis of a wide range of frequency bands.

The B&K Precision 2640 provides various functions and user-friendly interface which makes it easy to use. The handheld RF Field Strength Analyzer is ideal for users to test, install and maintain Mobile Telecommunications Systems, Cellular and Cordless Phone, CB Paging, Paging Systems, Cable and Satellite TV Systems as well as antenna site measurements and maintenance. The B&K Precision 2640 supports RS 232C serial communication and has separate GUI software. So, user can control the B&K Precision 2640 easily after connecting the B&K Precision 2640 with a personal computer, and can utilize the analyzed data variously after converting or saving numerical value or graph.

Features (section 2)

Main features

- 100 kHz to 2,000 MHz measurement range
- Frequency Spectrum Analyzing Function and Frequency Counter Function
- Measure N-FM, W-FM, AM, SSB signals
 N-FM
 W-FM
 A-MM
 SSB
- Demodulate W-FM signals
- Built-in 2 GHz Frequency Counter
- Accurate Signal Level Measurement
- Marker/Delta Marker/Squelch Adjustment Function
- PLL tuning system for precise frequency tuning
- Built-in Speaker
- 192 Pixels X 192 Pixels Back Light LCD
- Menu selection method for Function selection
- RS-232C Interface
- User-friendly Icon Display
- Maintenance of Wireless Telecommunications Equipments
- General Usage for Installation and Maintenance of Telecommunications Equipments
- Installation and Maintenance of Cable
- RFID Tag RF Strength Measurement
- Installation and Maintenance of Satellite Antenna
- Detection of Tapping and Hidden Camera

Functions (section 3)

RF Field Strength Analyzer

- Spectrum: Peak Search, Marker to Center,
- Internal Attn.: The input range can be extended by internal Max 10 dB Attn. function.
- Sweep Mode: Single Run, Free Run, Squelch Run Selectable
- Squelch Function: The Squelch Level may be adjusted to any value from the reference level to Full Scale.

Frequency Counter

- Frequency range: 35 MHz to 2,000 MHz
- No. of digits: 7 digits
- Resolution: 1 kHz

Frequency

Frequency Range	100 kHz to 2,000 MHz	
Resolution	Min. 6.25KHz Multiples	
Accuracy	± 4.5 PPM	
W-FM / N-FM / AM / SSB	Wide FM : Approx. 180 kHz @-6 dB Narrow FM : Approx. 12.5 kHz @-6 dB AM/SSB : Approx. 2.4 kHz @-6 dB	
Step Range	AM, SSB, Narrow FM : 6.25kHz, 12.5kHz Wide FM : 6.25~125kHz (Multiple of 6.25 kHz) 125~2500kHz (Multiple of 125 kHz)	
Span Range	AM, SSB, Narrow FM : 1MHz, 2MHz Wide FM : 1~20MHz (Multiple of 1 MHz) 20~400MHz (Multiple of 20 MHz)	
Frequency Selection Mode	Center, Start/ Stop, Span	

Amplitude

Measurement Range	-45 dBm to –110 dBm	
Average noise Level	Wide FM : -100 dBm Max. Narrow FM : -110 dBm Max. AM/SSB : -100 dBm Max.	
Amplitude Units	dBm, dBmV, dBuV	
Reference Level Accuracy	±3.0 dB (typical) @ 400KHz to 600KHz ±2.0 dB @ over 600KHz	
Reference Level Range	0 dBm to –80 dBm	
Log Scale	0.2 dB/DIV min, in 0.25 dB Span (5 Display Division)	
Internal Attn	10 dB	
Internal Attn Accuracy	±1.0 dB (@25 °C)	


Sweep	Speed	Min. 500 msec
	Trigger Source	Narrow FM / Wide FM / AM / SSB
	Trigger Mode	Free Run / Single Run / Continuous Wave / Squelch Run
	Trigger Level	TTL Level
	Marker Mode	Maker / Delta Maker
Memory	Trace & Setup Storage	Max 100 Waveforms and 100 States
Display	Туре	Mono STN LCD
	Display Resolution	192 Pixels X 192 Pixels
	LCD Light	On / Off
Frequency	Frequency Range	35 MHz to 2,000 MHz
Counter	Resolution	7 Digits
	Accuracy	±50 PPM ±1 COUNT
	Sampling Time	1 sec
	Input Sensitivity	35 MHz to 2,000 MHz : 150 mVrms
	Input Impedance	50 Ohms
	Max. Input Voltage	5 Vrms Max.

Spectrum	RF Input Connector	N type Female, 50 Ohms
input Port	Max Input Level	Max. +10 dBm, 5Vrms
DANGER		
Operation Environment	Operating Temperature	0 °C to 40 °C
	Humidity	35 RH to 85 RH
	Storage Temp.	10 °C to 50 °C
Power	Battery Power	AA Type Ni-MH Rechargeable Battery × 6
Source	Source	PCS
	Battery	AA Type 1.2 V, 2,700 mAh Rechargeable
	Specification	Nickel Metal Hydride Battery
DANGER	Adapter	SMPS Type AC Adapter (DC 12 V Output) Car-Adapter (DC 12 V Output)
	Auto Power On/Off	Off/ 5 min./ 10 min./ 20 min./30 min.
	Rechargeable Battery is controlled temperature of Battery Rechargeable Batter increased in some closes charging qu (dT/dt) of external te Battery protection, the in temperature sens be increased to mo temperature of Battery usage, it is strongly	2640 can be quickly recharged using Ni-MH eries. The Recharged method of Ni-MH d by the voltage of the Battery Cell and the ttery. The external temperature of Ni-MH ery is gradually increased and then quickly point of time. The B&K Precision 2640 ickly after checking the increased amount emperature of Battery for a unit time. Also, for he recharging is compulsory closed by built- or in case that the voltage of Battery Cell will re than some specified level or the external ery will be going up to over 50C. For safe recommended to use Ni-MH Rechargeable do not use in the place with high temperature ing recharging.

-

Physical	Dimension	4 "(W)×9 "(H)×1.8 "(D)	
Specifications	Weight	Approx. 0.66 Kg(1.45 lbm)	
		(including Antenna, except Battery)	
Standard Accessories	Antenna (Receive Only), SMPS Type AC Adapter, Fuji-AA type NI-MH		
Accessories	-	ry (6 PCS, 1.2 V 2,700 mAh), Manual, Coaxial	
		Carrying Case, Carrying Belt, RS-232C Cable, oftware for PC Application	
	Specifications and information	ation is subject to change without notice.	
	For the most current prod	uct information please visit www.bkprecision.com	

Instrument overview (section 4)

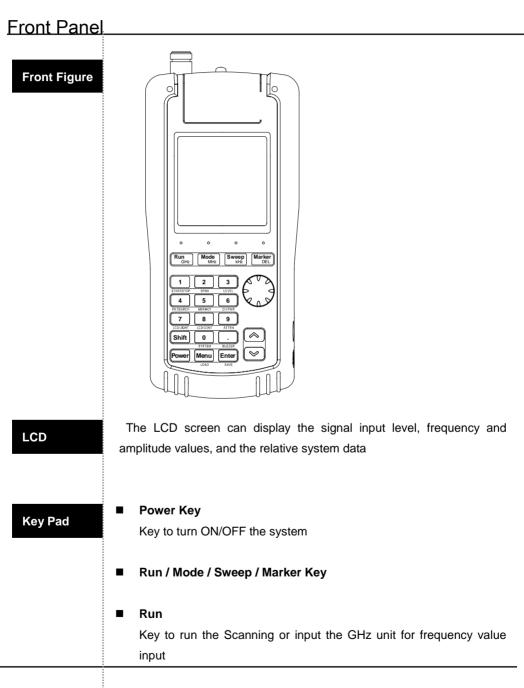

Front Panel

Mode

Key to set up the Reception Mode or input the MHz unit for frequency value input

Sweep

Key to set up the Sweep Mode or input the kHz unit for frequency value input

Marker

Key to select the Marker Function: Marker, Delta Marker, Squelch Marker, Peak Search and Marker to Center

Numeric Key

Key to input the frequency value

Menu Key

Key to set up the required functions of system

Up/Down Key


Key to select the Menu or Frequency Value

Knob Key

The function of **Knob** key is same as the **Up/Down** keys

Rear Panel

Rear Figure

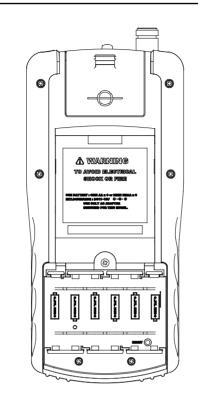

Belt Clip

User can yoke the B&K Precision 2640 on a belt.

Speaker

User can use the speaker to output the modulated audio from RF signal level.


Reset Key

User can use this Reset key for system malfunctions or memory reset.



Battery

Note the polarity of batteries at inserted battery compartment. And user must use the AA type Ni-MH Rechargeable batteries for battery charging

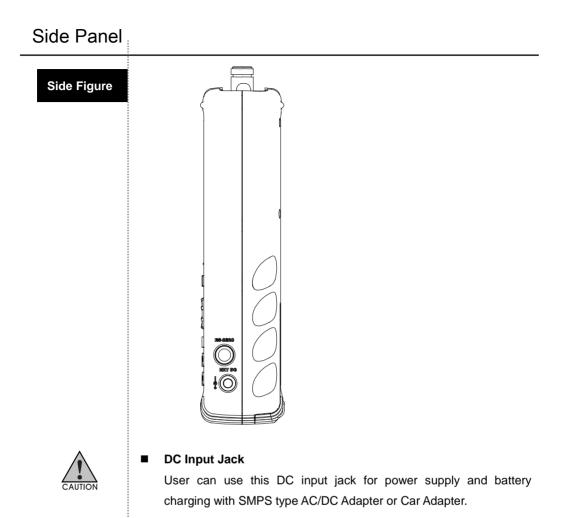


RS-232C Connector (8 pin mini DIN connector)

ł

User can use this RS-232C connector for PC communication with serial cable.

Top Panel

Top Figure



Input Connector for Signal Level

User can connect the antenna or coaxial cable to this connector on the system. The maximum input voltage is 5 Vrms.

■ Input Connector for Frequency Counter

User can connect the signal source to be measured to this connector. The maximum input voltage is 5 Vrms.

Volume Control

User can control the volume of audio output. To increase the volume of audio output, turn the Volume Control to clockwise direction.

Earphone Jack

Basic operation (section 5)

Before Power ON

How to insert and charge the AA Type Ni-MH rechargeable batteries? For the insertion of batteries, please release the screw on the battery cover on the bottom of the instrument. And put in AA Type Ni-MH rechargeable batteries (Total 6 PCS).

To charge the batteries after inserting batteries, connect the DC cable plug of SMPS type adaptor to DC jack of system (DC output: 12V).

Battery charging will begin after DC cable in connected.

At this time, if user turns on the power of system, the battery icon on the display window is displayed and blinking. And if the charging of batteries is finished, the blanking of battery icon will stop and only be displayed.

Connection for Input

Level

To measure the input level of RF signal, connect the antenna or coaxial cable to N-type connector of system (marked ANT)



Input Connector for RF Signal Level:

User can connect the antenna or coaxial cable to this connector on the system. The maximum input voltage is 5 Vrms

Input Connector for Frequency Counter:

User can connect the signal source to be measured to this connector. The maximum input voltage is 5 Vrms.

To turn on the system power, Press the Power key.

The system power is ON. The last displayed screen from the previous usage will be displayed (Previous setup status).

This system supports the simple manipulation with frequently used

function keys. To use this simple manipulation, push the shift key and push the numerical key. The frequently used function is marked on the numerical key below.

The upper right icons are the basic **2640** mode and the **SHIFT** mode. User can select the shift mode or basic **2640** mode by pressing the **Shift** key.

If the LCD screen is not readily visible, user can adjust the LCD contrast to see LCD screen.

To adjust the LCD contrast, push the shift key. And push the No. 8 (LCD Contrast) key. Until user's desired LCD contrast is adjusted, use the Up/Down keys and Knob key.


To turn on the LCD light, push the shift key. And push the **No. 7 (LCD** Light) 7 key. Then the LCD light is turned on.


And to turn off the LCD light, push the (shift) key. And push the **No. 7** (LCD Light) (7) key (Toggle ON/OFF).


For the LCD display, refer to below figure.

Turn on power of instrument


Power On	STEP 1
	- Push the ^{Power} Key.
	STEP 2 (Adjust to LCD Contrast)
	- Push the ^{Shift} Key.
	- Push the LCD CONTRAST (No.8) ⁸ Key.
	- Adjust to desired LCD Contrast using the Up/Down 🔊 🕙 Keys or Knob 🗘 Key.
	STEP 3
	- Push the Dot . Key and will be taken out of Menu.
	STEP 4 (LCD Light On/Off)
	- Push the Shift (Shift) Key
	STEP 5
	- Push the No. 7 (LCD Light) 7 Key

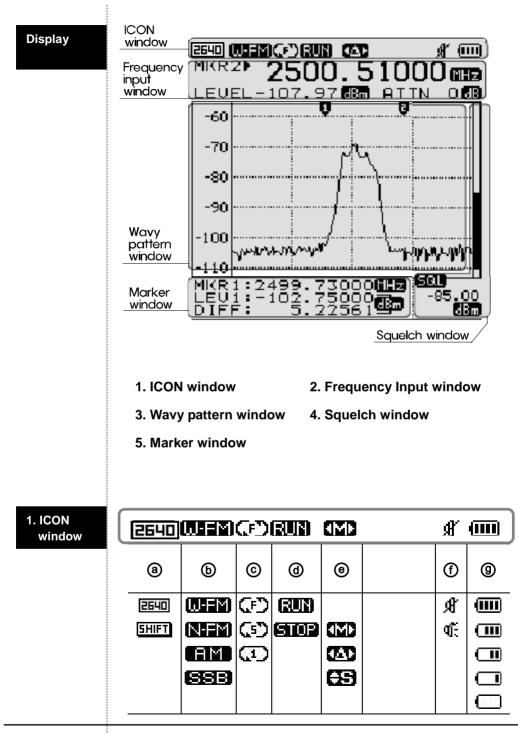

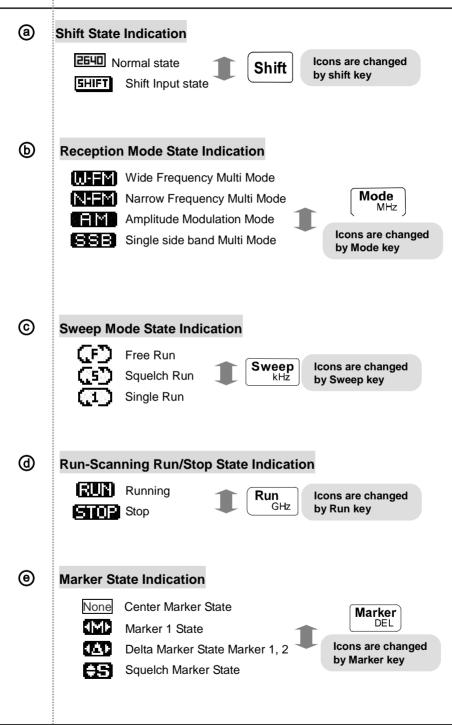

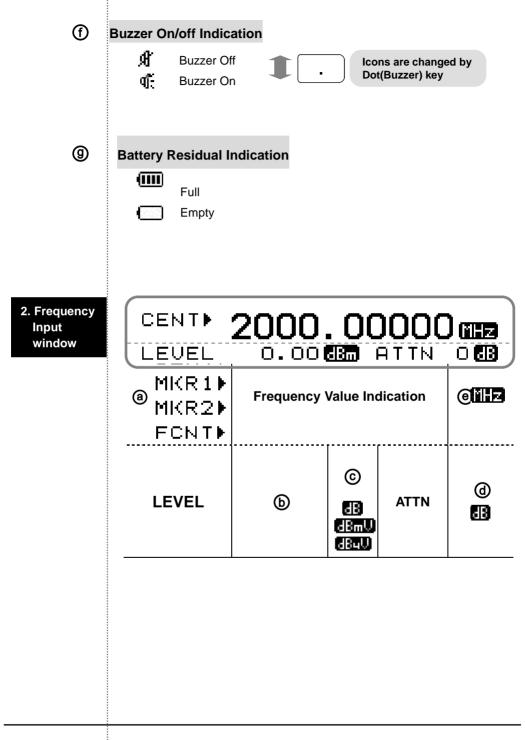


(3)	CENT Center Frequency Indication NONE MKR1 Maker 1 Frequency Indication M MKR2 Maker 2 Frequency Indication C FCNT Frequency Counter Value Indication Frequency Value of each Mode
Ь	Level Value Indication
	Indication of Level Value of each Mode
©	Level Unit dB dBmW dByW
	Can be established in Menu. [Please refer to Menu Level Unit establishment for further details]
Ø	Atten. Establish Value
	Indicate established Atten. Value. (Internal + External Atten. Value) [Please refer to Menu Level Unit establishment for further details]
0	Frequency Unit
	Every Frequency Unit is indicated in MHz

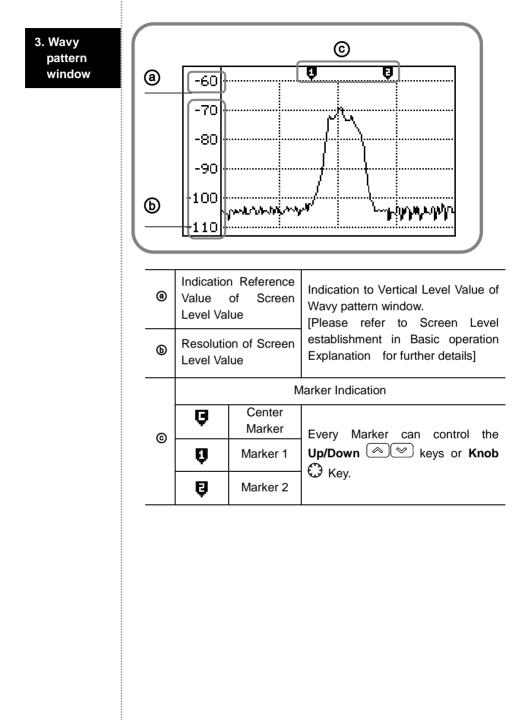

ł

4. Marker Window



(a) Center Marker, Marker 1, When Squelch Marker

CENT	Center Frequency	
SPAN	Span Frequency	MHz
STEP	Step Frequency	

b When Delta Marker

MKR1	Marker 1 Frequency	
LEV1	Marker 2 Level Value	i
DIFF	Marker1- Marker2 Level Value	dBm

Reception Mode

Wide-FM	Wide Frequency Modulation
	Wide FM RBW(Resolution Bandwidth) 180 kHz
Narrow-FM	Narrow Frequency Modulation
	Narrow RBW(Resolution Bandwidth) 12.5 kHz
AM	Amplitude Modulation
	SSB /AM RBW(Resolution Bandwidth) 2.4 kHz
SSB	Single Side Band Modulation
	SSB /AM RBW(Resolution Bandwidth) 2.4 kHz

Wide FM should be used to interpret a large Signal of Band width, Narrow FM should be used to interpret a narrow Bandwidth Signal. AM and SSB can used irrespective of Bandwidth.

Push Mode (MHz) Mode (MHz) Key to establish the reception mode and then the top-left ICON will be changed to WFM WFM, NFM NFM, AM

FIMD, SSB SSB order. When inputting Frequency like Start/Stop,

Span etc, the **Mode (MHz**) Mez Key is used.

RBW is fixed in each Mode as follows.

Wide FM RBW (Resolution Bandwidth) 180 kHz Narrow RBW (Resolution Bandwidth) 12.5 kHz SSB/AM RBW (Resolution Bandwidth) 2.4 kHz STEP 1

Reception Mode Establishment

- Push the Mode (MHz) Mode Key.

STEP 2

- Push the Mode (MHz) Key and t the top left ICON will change

to WFM (U-EM), NFM (N-EM), AM (EIM) and SSB (SSB) order.

Sweep Mode

Sweep Mode is used to set up operation characters which interpret Input.

Every each operation character is same as follows.

Free Run	Analyzing execution consecutively
1 Single Run	Only 1 time Execution
Squelch Run	Run by higher than Squelch level (Similar Trigger Mode of Oscilloscope)

Establish this mode by pushing the Sweep (kHz) ^{Sweep} Key and then the top left ICON will be changed to FREE Run **GP**, SQUELCH Run **GD** and SINGLE Run **GD** order. The Sweep (kHz) ^{Sweep} Key is used as input Start/Stop, Span and Input Frequency Unit into kHz Unit.

After input is finished Frequency, **FD** FREE Run continues to execute Run-Scanning operation automatically.

GD Squelch Run operation will stop Run-Scanning in case of Signal Level Value is getting higher than Squelch Level Value. But, If Signal Level is getting lower than Squelch Level, restart to Run-Scanning.

After input is finished Start/Stop Frequency, D Single Run execute Run-Scanning just a once. In addition, if it is desired to Run-Scanning, push the Run (GHz) (Run GHz) (Run GH

Sweep Mode Establishment

STEP 1

- Push the Sweep (kHz) Sweep Key

STEP 2

- Push the **Sweep (kHz)** Key, and the top-left ICON will be changed to **CFD** FREE Run, **CFD** SQUELCH Run and **CFD** SINGLE Run order.

Set up Span

The span is able to be set 1MHz to 400MHz. It has two settings – 1MHz step up to 20MHz and 20MHz step from 20MHz to 400MHz. If other numeral keys than MHz unit key is pushed, the input unit will be set to the nearest times by rising automatically.

Ex 1) When span input is 9.25Mhz, span will be 10MHz. Ex 2) When span input is 48MHz, span will be 60MHz.

First, push the **Shift** [Shift] Key (Shift icon is upside-down) in order to set up Span. The top-left ICON is changed **EFUD** to [SHIFT].

After that, push the Numerical Key. So then Frequency Input window changes the Span Input State.

Enter the Input Frequency and then input the Unit to use for this **Run** (GHz) \mathbb{R}^{Int} , Mode(MHz) \mathbb{M}^{Int} or Sweep (kHz) \mathbb{R}^{Int} Key would be set up Span.

Regardless of Frequency Input State, upper Keys are only used the input units.

STEP 1

Set up Span Mode

- Push the Shift Shift Key

STEP 2

- Push the No. 2 2 Key
- When the **Sweep (kHz)** ^{Sweep} Key is pressed, the top-left ICON is changed to **GFD** FREE Run, **GFD** SQUELCH Run and **GFD** SINGLE Run order.

Frequency Input

Chosen Reception Mode, Sweep Mode and Span are showed on the top center of LCD. At first, choose Reception Mode and Sweep Mode to get a sense of the Frequency Bandwidth and a specific feel for analyzing.

Choosing Frequency Value is a way to inputting Center and Start/Stop Frequency.

To order to input Center Frequency just pushes the numeral keys. Press the key when Frequency Input Window is a CENT state.

Push the **Shift** Shift Key to input Start/Stop Frequency.

Push the **Shift** (shift) Key to input Frequency you would like to analyze.

Push the **No. 1(Start/Stop)** ¹ Key, to inputted Start Frequency in Frequency Input Window.

Input Frequency by using the No. 0 to 9 Skeys, Dot (Buzzer) · Key, MARKER (DEL) Marker Key and Run (GHz) Runger as Unit Input Key, Mode (MHz) Mode and SWEEP (kHz) Key.

Execution will be done automatically, after inputting the last Unit in the Frequency, according to a given Sweep Mode of Run-Scanning Mode. If the mode is Single Run , push the **Run (GHz)** Key and then execute Run-Scanning again.


A wrong inputting content can be erased by using the **MARKER (DEL)** $\stackrel{\text{Marker}}{\overset{\text{Marker}}{\overset{\text{DEL}}}}$ Key operates like the Back space on PC

Inputting Frequency in out of Frequency Input Mode:

Frequencies can be deleted by pushing the **MARKER (DEL)** Key several times.

Erase inputted Frequency and then push the Marker (DEL) Key one more time, you are now out of Frequency Input Mode.

Frequency Input

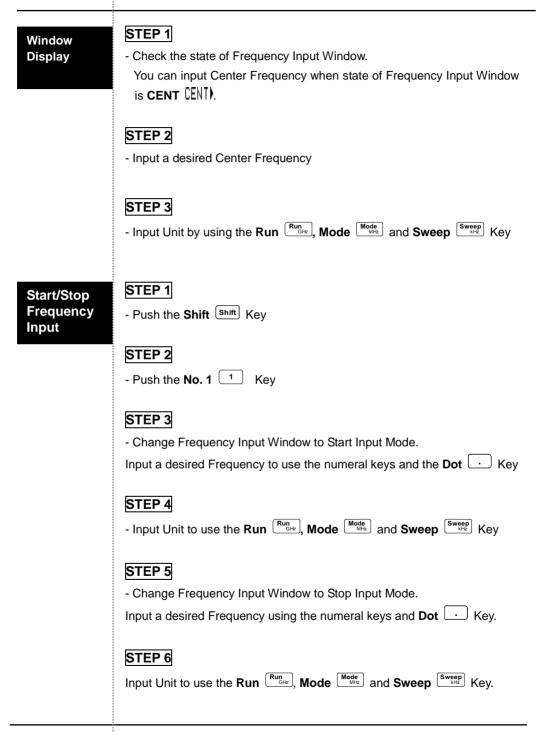

Adjust screen Level

Settle Top Level- Reference Level and Level Resolution to be Display or scene.		
"RLEV" is an abbreviation of Reference Level. Choose through the Up/Down < Keys and establish to use the Enter Enter Key. Top Level in verticality axis would be changed established Value.		
"DIFF" is an abbreviation of Difference. Choose through the Up/Down S Keys and establish to use Enter Key. Level Step in verticality axis would be changestablished Value		
RLEV Choose through the Up/Down C Keys and put the Enter Enter Key.		
DIFF Choose through the Up/Down C Keys and pu the Enter Enter Key.		
DIFF	-70 -70 -80 -90 -100 yww.v.h.Wi.wyW -110	

Run-Scanning

Run-Scanning is a process interpreting Frequency according to established Frequency Bandwidth and Span. And Run- scanning processes operate by establishing Sweep Mode




Run-Scanning process would be accomplished by establishing Reception Mode and Sweep Mode (See above)

ł

1

B&K Precision 2640 has Center Marker, Marker 1, Delta Marker (Marker1 and Marker2) and Squelch Marker. Each Marker Mode can define a state of Marker ICON into the top-left Marker Mode ICON.

Marker Mode ICON	Marker ICON	
Center Marker No ICON	Ģ	
Marker 1	Û	You can settle Marker 1 in this state.
Marker 2	Ô Ô	You can settle Marker 2 in this state.
Squelch Marker		Fix the volume when listening by making a multiple Signal to audible Frequency Bandwidth to use FM/AM/SSB and then fix Basic Signal of Squelch Run.

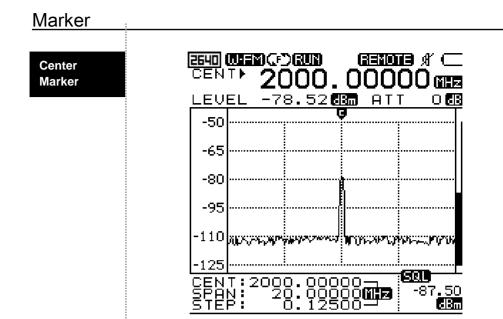


Center Marker is not a Mode the user will choose when using Mark Mode in Basic operation. When inputting Start Frequency and Stop Frequency, Center Frequency information will appear automatically.

The state is not indicated on the Mode ICON is Center Mode.

Frequency and Level on Center Frequency will be indicated on Frequency Input Window.

Marker

Marker 1

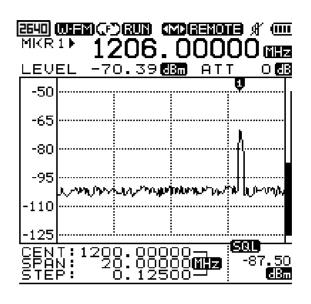

To use Marker 1 $\mathbb{M} \subseteq \mathbb{R}$ 1 , press the **Marker(DEL)** $\mathbb{M}_{\text{DEL}}^{\text{Marker}}$ key in Center Marker status. When it turns to Marker 1 mode, Marker mode icon is changed to \mathbb{M} . And frequency input window is changed to Center Marker to Marker 1 $\mathbb{M} \subseteq \mathbb{R}$ 1 .

To move the Marker 1, use the **Up/Down** > we keys, or the **Knob** > keys. Then the frequency value and level value are displayed on frequency input window


STEP 1

- Press the Marker (DEL) ^{Marker}_{DEL} Key.
- Check the Marker 1 MM mode in display window

STEP 2

- To move the Marker 1 to wanted plot point, please use the **Up/Down**
- Then the frequency value and level value are displayed in the frequency input window

Marker

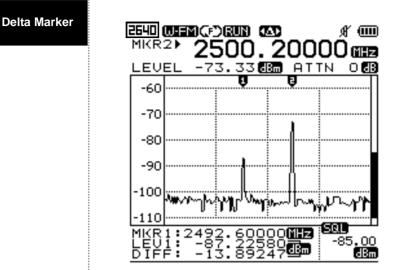

Press the **Marker (DEL)** Key until the Marker mode icon is changed to Delta Marker **Marker** in the display window. And in this case, Marker 2 is added.

The Marker mode is the total four modes. And the changed order of Marker mode is as below:

Center \rightarrow Marker 1 \rightarrow Delta Maker \rightarrow Squelch Marker



To handle the Marker 1, user can set up the marker 1 in Marker mode 1 To handle the Marker 2, user can set up the marker 2 in Delta Marker

When user set up the Delta Marker, the frequency value and level value of Marker 2 are displayed in the frequency input window. The frequency value and level value of Marker 1, and the difference level value between Marker 1 and Marker 2 are displayed in the Marker window


STEP 1

- Press the Marker (DEL) Marker (DEL) Key.
- Check the Delta Marker from mode in the display window

STEP 2

- To move the Marker 1 to wanted plot point, please use the **Up/Down**
- Then, the frequency value and level value of Marker 2 are displayed in the frequency input window.

The frequency value and level value of Marker 1, and the difference level value between Marker 1 and Marker 2 are displayed in the Marker window. Then the frequency value and level value are displayed in the frequency input window

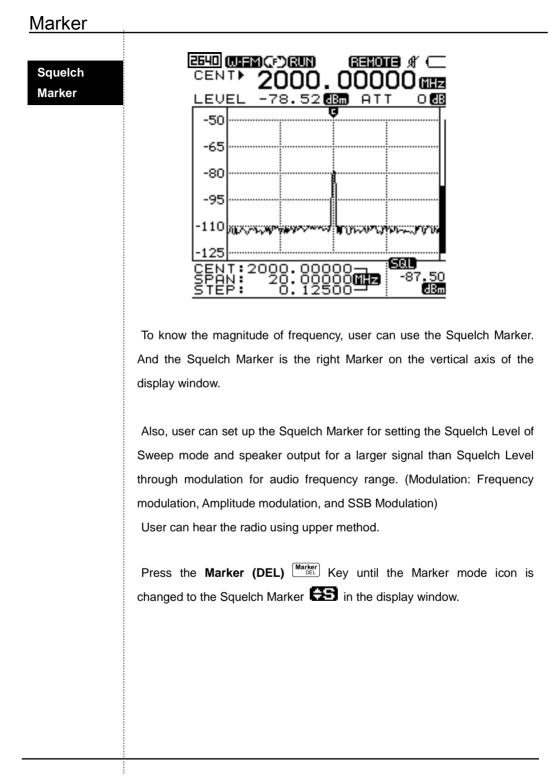

STEP 1

- Press the Marker Marker key.
- Check the Squelch Marker 🖽 mode.


STEP 2

- Move the Squelch Marker to wanted point using the Up/Down
- Keys or **Knob** 🛈 Key.
- The squelch value is displayed in the lower right display window.



Power Meter

Single Power Meter Function



To use the Single Power Meter Function, at first push the **Shift** $(2^{\mu_{\text{H}}})$ and then check the icon that is changed.

Please push the numeral 4(Single) key. After inputting the frequency to measure, input the unit.

STEP 1

- Push the Shift Shift Key.

STEP 2

- Push the NO.4(SINGLE) 4 Key.

STEP 3


- Input the frequency to measure ...

STEP 4

- Input the units using **RUN** (Run GHZ), **Mode** (MHZ) and **Sweep** (kHZ) keys.

Power Meter

Multi Power Meter Function



To use the Multi Power Meter Function, at first push the **Shift** (shift) key and then check the icon that is changed.

Please push the **No. 5(MULTI)** key. Assign any number of frequencies to measure within 1 to 9. After inputting the frequency to measure, input the unit.

STEP 1

- Push the Shift Shift Key.

STEP 2

- Push the No.5 (MULTI) 5 key.

STEP 3

- Input a number within 1 to 9

STEP 4

- Input frequency to measure.

STEP 5

- Input the units using **RUN** ^{Run}_{GHz}, **Mode** ^{Mode}_{MHz} and **Sweep** ^{Sweep}_{KHz} keys.

UNIT

UNIT Change Function



STEP 1

- Push the Shift Shift Key.

STEP 2

- Push the No.6 (UNIT) key.

STEP 3

- Using the **Up/Down** (Key or **knob** (key, move to the measuring unit and then set up by **Enter** (**Enter**) key.

÷

Setting of Attenuator

Setting for Internal or External	The internal attenuator is used for maximum input signal -45dBm with Menu function. To set the internal attenuator, press the Shift Shift key to change the upper right icon EGUD to SHIFT. And press the No. 9 (ATTN) (a) key. To adjust the value of internal attenuator, press the Up/Down (c) (c) Keys or rotate the Knob (c) key. And Press the Enter Enter key.
	If the input signal is larger than -20dBm (ex10dBm, 0dBm, and etc), user can use the user's external attenuator.
	Setting of the EXT. ATTEN. is as below Push the No. 9(ATTN) ● key. INT. ATTEN in system is set up. Push the Dot • key and then move the previous menu. After selecting the EXT ATTEN using the Up/Down ● W Image: Set up. Push the Dot • key and then move Image: Set up. Push the Dot • key and then move Image: Set up. Push the Ext attent using the Up/Down • W Image: Setup the Set

The LCD Light is designed to ease the use of the instrument in a dark location.

Press the Shift Shift key to change the upper right icon 2640 to SHIFT.

And press the No. 7 (LCD Light	:) [7	key
--------------------------------	-------	-----

*The Power ON/OFF of the LCD Light is toggle

STEP 1

- Press the Shift Shift key

STEP 2

- Press the No. 7 (LCD Light) 7 key



If the LCD light is ON, the current of battery is relatively larger than when LCD light OFF. In other words using time of system is shorter

LCD Contrast



The function of LCD contrast is to adjust the contrast for the remained battery capacity.

Push the Shift Shift key to change the upper right icon 2640 to SHIFT.

And push the No. 8 (LCD Contrast) ⁸ key.

The LCD contrast is adjusted by using the **Up/Down** O keys or **Knob** O key. And push the **Enter** key.

STEP 1

- Press the Shift Shift key

STEP 2

- Press the No. 8 (LCD Contrast) 8 key

STEP 3

- To adjust the LCD contrast, use the $\mbox{Up/Down}$ $\textcircled{\mbox{\sc blue}}$ keys or \mbox{Knob}
- key and press the Enter key

Buzzer ON/OFF

 User can set the Buzzer ON/OFF (Toggle ON/OFF) Push the Shift Shift Key. Then the Icon EFID of left upper window is
changed to shift icon EHIFT . And press the Dot · Key.
And press the Dot . Key.
 STEP 1 - Press the Shift ^{Shift} key
 STEP 2 - Press the Dot · Key

.

The function of Save/Load is for the Waveform and Setup Statuses.


The function of Save is for concurrently saving the Waveform and Setup Status in memory.

And the saved Setup Status in memory includes the following information: Reception mode, Sweep mode, Frequency range, Step value, and Span value. User can use this with Menu or Multi key.

The function of Load is for loading the saved Waveform and Setup Status in memory.

If user only wants the Setup Status, please load the saved file for desired Setup Status. And press the Run key. Then this measuring instrument will complete the Run-scanning operation. User can only use this in Menu.

The function of Delete is for deleting the saved file. Also User can only use this in the Menu.



Save

STEP 1

- Press the Shift shift key

STEP 2

- Press the Enter Enter key

STEP 3

- To save the waveform or setup status, a name with at least 7 characters is required.

- To select the first character. Use the **Up/Down** keys. And press the **Enter** key

- If want to save the file name fewer than 10 characters, press the "END' on stated inputted file name.

STEP 4

- To delete the character, press the Marker Marker key

STEP 5

- When all 7 characters included blank are typed, press the **Enter** key. Then, output message for SAVE OK is displayed.

"SAVE OK"

- If user does not type the all 7 characters included blank, the function of save is not completed


STEP 6


- To cancel the Save, press the **Marker** ^{Marker} key until the first character is deleted. And additionally press the **Marker** ^{Marker} _{DEL} key one time.
- Then the Save is canceled and the output message is displayed as below.

"SAVE FAILED"


- The values to be saved are signal and system setting values. Buzzer,

LCD contrast and LCD light states are not saved.

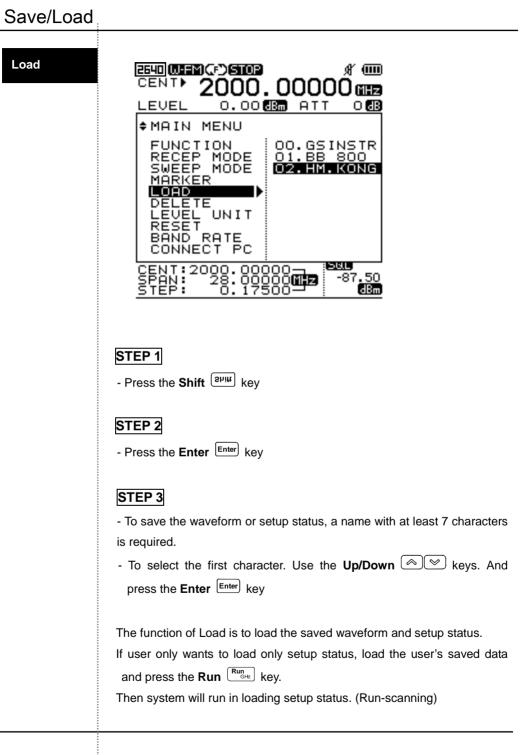

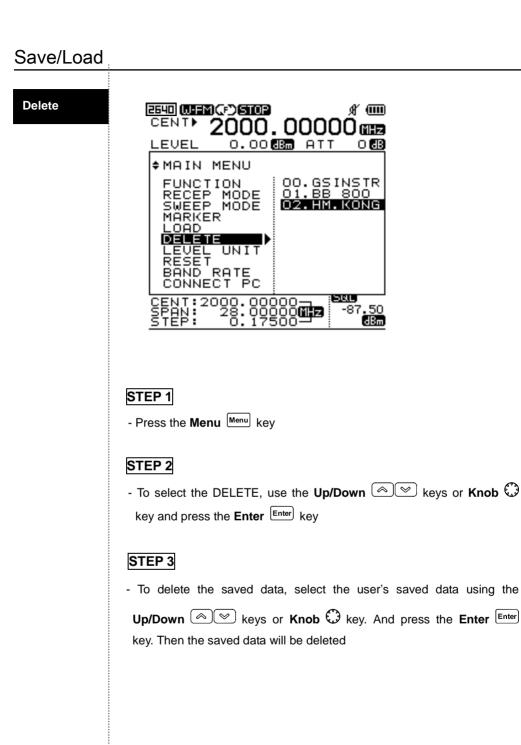

Frequency Counter



Select the F.counter under Main Menu - function

The input connector for the frequency counter is BNC connector. When the input level is inputted into the Frequency Counter, the measured frequency value is displayed in the frequency input window

Input level is same as below.

35 MHz to 2,000 MHz : 150m Vrms 20 MHz to 1,000 MHz : 100m Vrms



Frequency Counter

STEP 1

- Press the Menu Menu key

STEP 2

- To select the FUCTION, use the **Up/Down** keys or **Knob** keys or **Knob** keys or **Knob**

- Then sub menu is opened.

STEP 3

- To select the F. COUNTER (Frequency Counter), use the **Up/Down**

STEP 4

- The icon **EEEE** is displayed from the other icon.

The FCNT is displayed in the frequency input window

STEP 5

- When the input level is inputted in the Frequency Counter using BNC connector, the measured frequency value is displayed in the frequency input window

STEP 6

- To change the Frequency Counter mode to Spectrum mode, run the upper Step 1 to Step 3. At this time, select the SPECTRUM not F. COUNTER in **Step 3**

Power Source

Checking for Battery

To check the battery's remained capacity Battery, user can refer to the battery icon in the upper area of display window



How to use and replace the battery

The power system of B&K Precision 2640 uses the Ni-MH rechargeable batteries. Then, the power system supports fast charging. The charger for the Ni-MH batteries is controlled by the voltage and temperature of the battery cells.

The Ni-MH rechargeable batteries must be used for the safe and stable power source. And if the charging is required, please avoid the site with high temperature or high humidity

Level Unit

Setting of the Unit

The setting for level unit can be set up in the Menu.

The level unit can be set up as below

□ dBm

- □ dBuV
- \Box dBmV

STEP 1

- Push the Menu Menu key

STEP 2

- To select the LEVEL UNIT, use the **Up/Down** keys or **Knob** key and push the **Enter** key. Then sub menu is opened.

STEP 3

- To select the user's wanted level unit, use the Up/Down region keys

or **Knob** (b) key and push the **Enter** key

The function of Reset is for initializing the memory or system.

The three kinds of resets are supported. And these resets are run through the Menu

Preset

System Reboot for initial setup status. (Center Frequency, Span Frequency, Marker and etc)

• Memory CLR

The user's saved data will be cleared. (Memory Cleared)

System INIT

The upper two resets (PRESET and MEMORY CLR) are run.

Then, system reboot for initial setup status and the user's saved data will be cleared

STEP 1

- Push the Menu Menu key

STEP 2

- To select the RESET, use the **Up/Down** > keys or **Knob** > keys and push the Enter Enter key.

- Then, sub menu is opened.

STEP 3

- To run the wanted Reset, use the Up/Down $\textcircled{\begin{times} \begin{times} Up \end{times} \end{times}$

key and push the Enter $\begin{tabular}{c} \mbox{Enter} \end{tabular}$ key.

- Then, the selected reset will be run

Baud Rate

Setting of
the BaudThe setting of the baud rate is for the transmission speed.
The Baud Rate between PC and system is same as below.Rate115,200 BPS (Default)57,600 BPS

38,400 BPS 19,200 BPS 9,600 BPS 4,800 BPS

STEP 1

- Push the Menu Menu key

STEP 2

- To select the BAUD RATE, use the **Up/Down** relation keys or **Knob** where the **Enter** key. Then, sub menu is opened.

STEP 3

- To select the wanted baud rate value, use the **Up/Down** (A) where we have been selected by the selected baud rate value, use the **Up/Down** (A) where the **Up/Down** (A) w

Connection for PC

Setting of
the
Connection
for PCThe function of CONNECT PC is for connecting to a PC.First, the GUI program is run on the PC. And the serial cable is connected
between PC and B&K Precision 2640.
Next, run the REMOTE PC from Menu.• NONE

• REMOTE PC

STEP 1

- Press the **Menu** key

STEP 2

- To select the CONNECT PC, use the **Up/Down** result were select the **Enter** key. We want press the **Enter** key. Then, sub menu is opened.

STEP 3

- To select the REMOTE PC, use the Up/Down 🔊 🔊 keys or Knob

G key and press the Enter key.

Then, the connection between the PC and the system is running.

Auto Power

The Auto Power function should be used to conserve system power. When the power OFF time is enabled ("NONE" is not selected), the power source will be turned off automatically if the user dose not use the system for the auto power OFF period of time.

The auto power OFF time is same as below

NONE 05MINUTES 10MINUTES 20MINUTES 30MINUTES

STEP 1

- Push the **Menu** Menu key twice

STEP 2

- To select the AUTO POWER, use the Up/Down 🔊 🖤 keys or Knob

key and push the **Enter** key.

Then, sub menu is opened.

STEP 3

- To select the auto power time, use the **Up/Down** keys or **Knob** key and push the **Enter** key

Level Offset compensates for any loss due to the cabling. Offset adds the value of +Offset to all values of measurement.

STEP 1

- Press the Menu Menu key twice

STEP 2

- Move the cursor on PC Connect using the Up/Down $\textcircled{\begin{times}{ll} \begin{times}{ll} \begin{times$


STEP 3

- Push the **Enter** Enter Key and then move the submenu.
- Move the dB value of Offset.
- Push the Enter Enter Key

STEP 4

- Push the Menu Menu Key one more time to exit the System

Menu

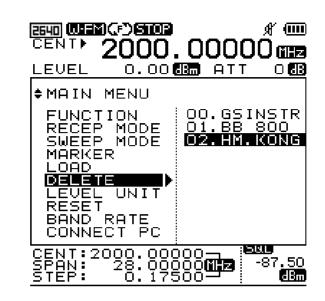

There are two modes. One is Multi key function with the **Shift** (2) Key and the other is to select other functions.

It can select the functions using multi key and in Menu.

The functions that could be selected in Menu mode is as blow

Level Unit

Reset

Band Rate

Connect PC

To exit from Menu or System, push the **Menu** Menu Key or push the Dot key. These keys will move through the menu either lower or higher.

STEP 1

- Push the **Menu** Menu key twice

STEP 2

- To select wanted function, use the Up/Down Keys or the Knob Key.

STEP 3

- Push the Enter Enter Key

STEP 4

- After selecting function of lower item or On/Off, push the Enter Enter Key

STEP 5

- Exit the Menu after pushing the **Menu** Menu Key twice.
- When the $\textbf{Menu} \ \underline{\mbox{Menu}}$ Key is pushed one time, you are in System

Menu

-	Spectrum	 Set up the functions of Spectrum and frequency
	Frequency Counter	
Function	TEST Mode	counter. (note: TEST
	Single Power Meter	Mode is for Factory use — only)
	Multi Power Meter	<i>y</i>)
-	N-FM	Set up the Reception — Mode.
Reception	W-FM	It's possible to set up with
Mode	SSB	the Shift ^{Shift} Key (Shift button is upside-down
	AM	please check all buttons to confirm they are correct.)
Sweep	Free Run	Set up the Sweep Mode.
Mode	Squelch Run	It could be set up with the
mode	Single Run	Shift ^{Shift} Key.
-	None	Marker or function using
Marker	Marker	the Marker.
	Delta MKR	The mode can be set up
	Squelch MKR	with the Shift Shift Key.
Save	Save Data	The mode can be set up with the Shift Shift Key.
Load	Load Data	The mode can be set up with the Shift Shift Key.
	dBm	
Level Unit	dBuV	
	dBmV	

-

Menu

ł

.....

	Pre Reset	Restarting the System and clear all parameters for set up
Reset	Memory CLR	Delete the stored data
Reset	System INI	All Reset – restarting the system and delete the stored data
	115,200 BPS	
	57,600 BPS	
Dand Data	38,400 BPS	Select the speed of serial communication between the unit and PC
Band Rate	19,200 BPS	
	9,600 BPS	
	4,800 BPS	
Connect	None	Select the connection to PC
PC	Remote PC	

System



There are modes that select the function of Multi key using the **Shift** (shift) Key and the other functions.

Functions can be selected using the multi key and the Menu.

The functions that can be selected in Menu mode are as blow.

To exit from Menu or System, push the Menu Key or push the Dot key, this will move you to lower menu items or to higher menu items.

STEP 1

- Press the Menu Menu Key

STEP 2

- Press the **Menu** Menu Key once more.

STEP 3

- To select desired function, use the Up/Down $\textcircled{} \otimes \textcircled{} \otimes$ Keys or the Knob Key

STEP 4

- Press the Enter Enter Key

STEP 5

- After selecting a lower item function or On/Off, push the Enter Enter Key

STEP 6

- Push the Menu Menu Key once to exit the System

System

Auto Power	None 05 Minutes 10 Minutes 20 Minutes 30 Minutes	Select auto power saving mode.
Buzzer	ON OFF	Select Buzzer On/Off. It could be set up with the Shift Shift Key (Shift Key Icon is upside down. Please check all icons to fix this.)
LCD Light	ON OFF	Select LCD Light On/Off. It could be set up with the Shift Shift Key.
LCD Contrast	1 to 10 Step	
INT. Atten.	0 dB 10 dB 20 dB 30 dB 35 dB	
EXT. Atten.	0 dB to 90 dB	
Offset	-99.0 dB to 99.0 dB	
Default save	SAVE	During booting, save default value to be applied. When Saving the values, all values will be saved except Signal.

Description of key operating (section 6)

Run GHz

Run [GHz]


Instruction to start scanning frequencies


After power on, this button will work as it did under the most recent setup, or when Squelch Run **C** or Single Run **C** functions are active.

[Please refer to the Scan in description of basic operation details if needed]

• Units input function can be used to set up Start/ Stop/ Scan/ Center frequencies.

After inputting the frequency values, push the k GHz key to view the units.

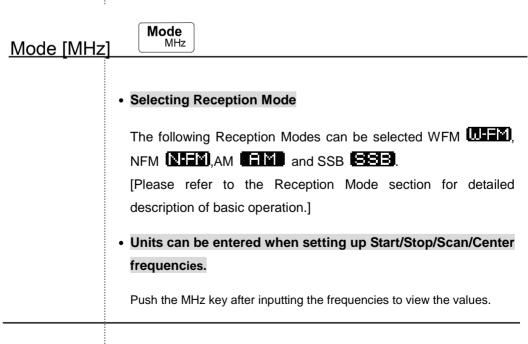

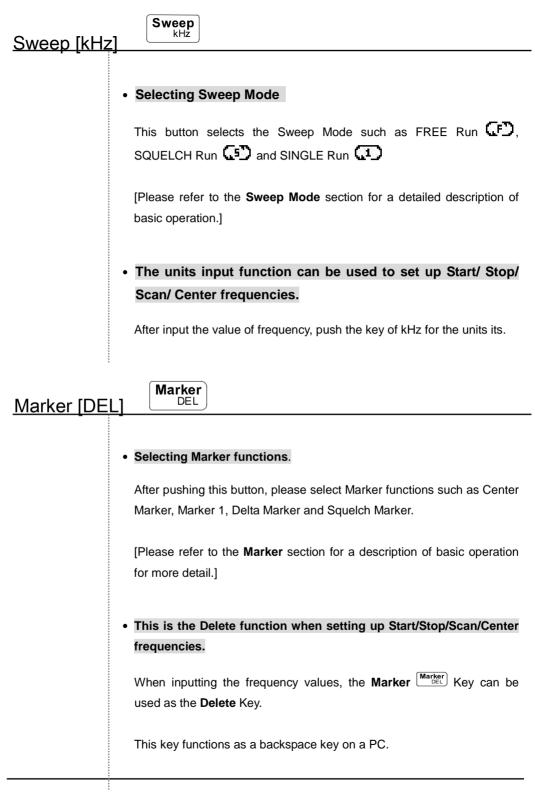


No. 1 [Start	/Stop]		
E	 Press the No. 1 <a>1 key to input the value of 1. To input the value of numeral 1 in the Start/Stop/Scan/Center frequencies, please use the No. 1 <a>1 Key. 		
• Pressing No, 1 key and the Shift Shift Key will active the			
Input function for Start/Stop Mode.			
	Select the Start/Stop Mode by pushing the Shift Shift Key and than push the numeral 1 Key.		
	[Please refer to the Frequency Input section for a description of basic operation if more detail is needed.].		
<u>No. 2 [Spar</u>	<u>]</u> 2		
	 Press the No. 2 ² key to input the value of 2. 		

Input the value of numeral 2 in the Start/Stop/Scan/Center Mode by pressing the **No. 2** $\stackrel{2}{=}$ Key.

 Span Frequency Input function can be activated by pushing Shift Shift Key

By pushing the **Shift** Shift Key and than pushing the **No. 2** Key, the Span Mode can be activated.

[Please refer to the **Span** section for a detailed description of basic operation if required.]

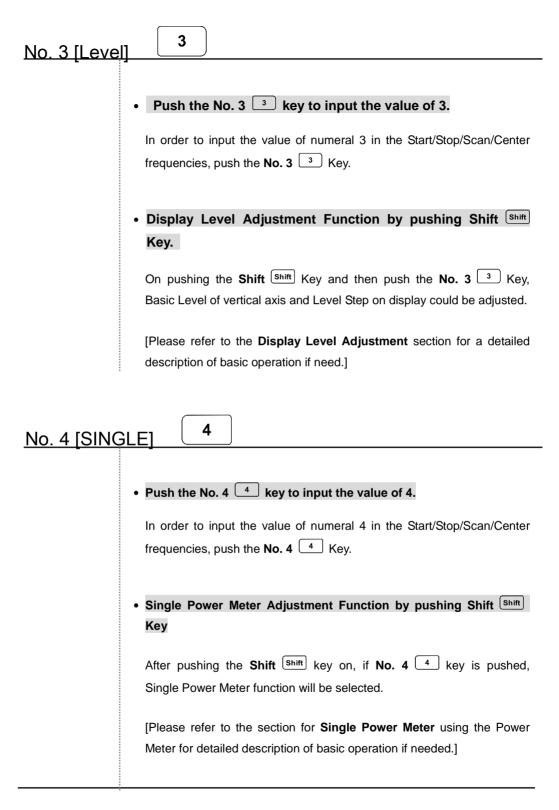

No. 5 [MUL	TII	5	
L	Pusl	n the No	 o. 5 ⁵ key to input the value of 5. o. 5 ⁵ Key to input the value of numeral 5 in the Start/ Center frequencies.
	• Muli Key		r Meter Adjustment Function after pushing Shift Shift
		-	the Shift shift key and then pushing the No. 5 key is Iti Power Meter function can be selected
	_		er to the Multi Power Meter section for a details description e Power Meter if needed.]
No. 6 [UNIT	-]	6	

• Push the No. 6 6 key to input the value of 6.

The **No. 6** ⁶ Key is used to input the value of numeral 6 in the Start/Stop/Scan/Center frequencies.

Level Unit Adjustment Function after pushing Shift Shift Key

By pushing the **Shift** (Shift) key and then pushing **No.6** (6) key, Level Unit function can be selected.

[Please refer to the **Level Unit** section for a detailed description of basic operation if needed.]

No. 7 [LCD Light]

• Push the No. 7 7 key to input the value of 7.

When inputting the value of numeral 7 in the Start/Stop/Scan/Center frequencies, the **No. 7** 7 Key is used

LCD Light Function after pushing the Shift Shift Key

By pushing the **Shift** shift key and then pushing the **No. 7** Key, LCD Light function can be selected.

[Please refer to the **LCD Light** section for details about basic operation if needed.]

No. 8 [LCD CONT; LCD Contrast]

• Push the No. 8 ⁸ key to input the value of 8.

To input the value of numeral 8 in the Start/Stop/Scan/Center frequencies, the **No. 8** B Key is used.


8

LCD Contrast Function after pushing the Shift Shift Key

By pushing the **Shift** shift key and then pushing the **No. 8** Key, LCD Contrast function can be selected.

[Please refer to the LCD Contrast section for details on basic operation.]

9 No. 9 [Attenuator] • Push the No. 9 9 key to input the value of 9. To input the value of numeral 9 in the Start/Stop/Scan/Center frequencies, the **No. 9** • Key is used Attenuator Setup Function after pushing the Shift shift Key By pushing the **Shift** Shift key and then pushing the **No. 9** 9 Key, Attenuator function can be selected. [Please refer to the Attenuator Setup section for details about basic operation.] 0 No. 0 [System] • Push the No. 0 • key to input the value of 0. When inputting the value of numeral 0 in the Start/Stop/Scan/Center frequencies, the **No. 0** • Key is used. System Setup Function after pushing the Shift Shift Key By pushing the **Shift** (^{shift} key and then pushing the **No. 0** (⁰ Key, System Setup function can be selected. [Please refer to the System Setup section for details about basic operation.]

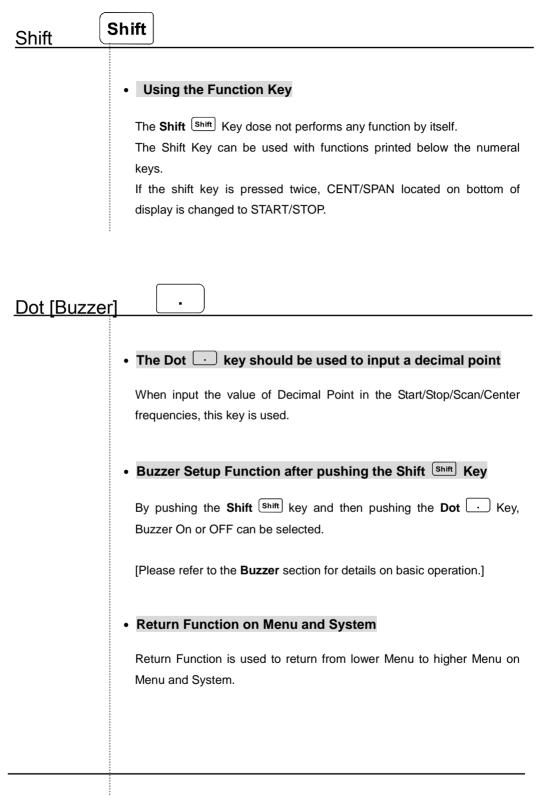

Menu [Load]

Menu Function

Various functions can be selected after entering Menu item.


At the Menu item, pushing the **Menu** Menu Key once more; will activate the System item.

[Refer the section of **Menu and System** of basic operation if need more detail]

• Load Function after pushing the Shift Shift Key.

By pushing the **Shift** shift key and then pushing the **Menu** Key, stored Data can be loaded.

[Please refer to the Store Mode section for details of basic operation.]

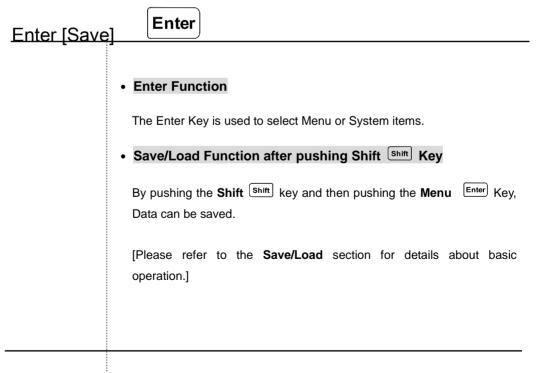

Up/Down Keys and Knob Key



• Up/Down 🔊 🗢 Keys and Knob 🛈 Key Functions

Movement of Marker, Menu items and System After setting the Span, the Span can be changed using the Up/Down key. After setting the Reference level, the Reference level can be changed using Up/Down key.

Service Information

Warranty Service: Please return the product in the original packaging with proof of purchase to the address below. Clearly state in writing the performance problem and return any leads, probes, connectors and accessories that you are using with the device.

Non-Warranty Service: Return the product in the original packaging to the address below. Clearly state in writing the performance problem and return any leads, probes, connectors and accessories that you are using with the device. Customers not on open account must include payment in the form of a money order or credit card. For the most current repair charges please visit www.bkprecision.com and click on "service/repair".

Return all merchandise to B&K Precision with pre-paid shipping. The flat-rate repair charge for Non-Warranty Service **does not** include return shipping. Return shipping to locations in North American is included for Warranty Service only. For overnight shipments and non-North American shipping fees please contact B&K Precision.

B&K Precision 22820 Savi Ranch Parkway Yorba Linda, CA 92887 www.bkprecision.com 714-921-9095

Include with the returned instrument your complete return shipping address, contact name, phone number and description of problem.

Printed in Korea

Copyrights © B&K Precision Corp. 2010

B&K Precision Corporation 22820 Savi Ranch Parkway Yorba Linda, CA 92887 www.bkprecision.com